

253710 Power Analyzer PZ4000

NEW



PZ4000 (253710)
426 × 177 × 450mm 15kg
(16.77 × 6.97 × 17.72" 33lbs)




★ Safety Standard; EN61010-1, CAT II, Pollution degree2
EMI Standard; EN55011 Group 1 Class A
Immunity Standard; EN50082-2 : 1995


The PZ4000 is a power analyzer based on a new set of concepts and designed for R&D work relating to environmentally friendly energy-conserving products and technologies. These products and technologies were the focus of the Third Conference of the Parties to the United Nations Framework Convention on Climate Change (COP3; held in Kyoto in December 1997), and are rapidly being adopted around the world. In order to support R&D for these products and technologies, the PZ4000 was designed based on YOKOGAWA's Environmentally Harmonious Product Design Guidelines and Product Design Environmental Assessment Standards, which are intended to protect the global environment. The PZ4000 has been developed and produced at ISO14001-approved offices.

FUNCTIONS

- A POWER METER THAT DISPLAYS MEASURED WAVEFORMS**
 Measured voltages and currents are sampled at high speed (maximum 5 MS/s). Power is calculated from the sampled data along with accurately displayed waveforms.
- Correlation between displayed waveforms and calculated power values**
 Waveform displays and calculated values (e.g., power values) are based on sampled data stored in internal memory, so they are correlated with each other.
- Check measurement effectiveness easily**
 Measured waveforms and calculated values can be checked at the same time to prevent erroneous measurements.
- No probe needed for waveform measurements**
 Voltage and current waveforms can be measured without using oscilloscope isolation probes and differential probes. The PZ4000 can make waveform measurements much more accurately than with conventional oscilloscopes.

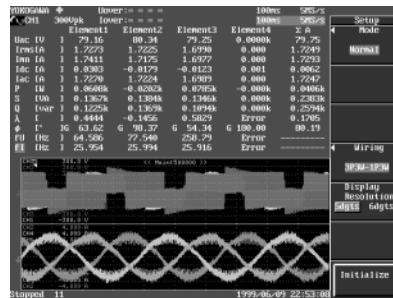

Example of output signal check for an inverter-driven 3-phase motor

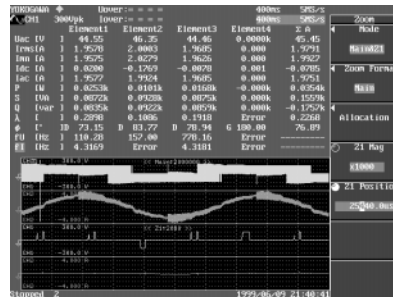

Example of check using zoom function to determine whether pulse waveforms are fully acquired during low-rpm operation

FEATURES

- Wide measurement bandwidth (DC, up to 2 MHz)**
- Accurately capturing of input waveforms using high-speed (maximum 5 MS/s) sampling**
- Voltage and current waveform display and analysis functions to enable power calculations on fluctuating inputs**
- Harmonic analysis (up to 500th order) and Fast Fourier Transform (FFT) functions to enable high-frequency power spectrum analysis**
- Simultaneous measurement of many channels using multiple units and external trigger function**
- Environmentally friendly design based on YOKOGAWA's "Guidelines for Designing Products for the Environment" and "Criteria for Environmental Assessment in Product Design."**
- WIDE BANDWIDTH, HIGH-PRECISION MEASUREMENTS**
 Measurements can be made over a wide frequency range (DC up to 2 MHz), making it possible to measure power loss on electronic components, high-frequency lighting equipment, and other devices.
- High precision power measurements at high frequency**
 The PZ4000 lets you make high-precision measurements of voltage, current, and consumed power in equipment driven at frequencies ranging from several tens of kHz to approximately 100 kHz.
- Lamp current measurement in fluorescent bulb**
 With the PZ4000, you can measure lamp current of fluorescent bulb using Delta Computation function. It computes the difference of the instantaneous values between output current of electric ballast and cathode current.
- Loss measurement when actual load is applied to electronic components**
 With the PZ4000, you can measure power loss resulting from actual load applications, instead of evaluating characteristics


PZ4000

based on small signals using an LCR meter or impedance analyzer.

- Power measurements on extremely low-frequency signals**
 Take full advantage of the 4M word internal memory (optional; enough for 4 million samples) to obtain precise measurements of extremely low-frequency signals (several mHz) signals.



Example of measurements on inverter lighting equipment with a fundamental wave of approximately 50 kHz

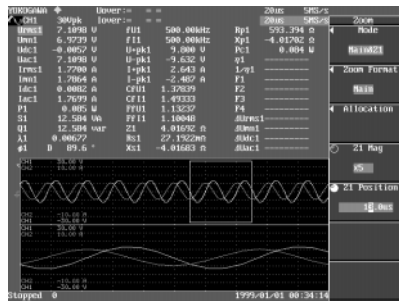


Example of loss measurement during high-frequency capacitor driving (500 kHz)

- A POWER METER CAPABLE OF DYNAMICALLY CAPTURING LOAD FLUCTUATIONS**

Internal memory (maximum 4 M words) stores your measurements. You can calculate and display voltage, current, and power values for specific portions of the total memory (equivalent to 100 k words of data). The display makes it easy to see how the load fluctuates with time.

- Inrush current and power measurements (at switch-on)**

In the past, it was necessary to measure inrush current and power values at power-on using measuring instruments such as oscilloscopes. The PZ4000 makes these measurements much more accurately and greatly simplifies this procedure.

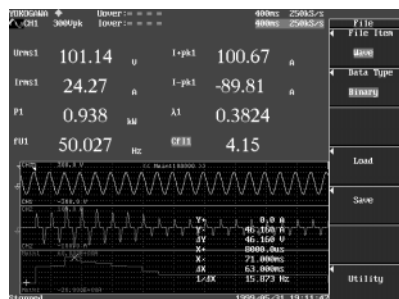

Example of inrush current measurement in an inverter-type cleaner

- Power measurements in specific states (specific spans in internal memory)**

Power measurements on equipment with fluctuating loads are normally obtained by measuring the energy in certain operating patterns over a long time period using an integration function. The average power value is then calculated. In contrast, The PZ4000 lets you make power measurements over a specific period defined by adjustable cursors. This reduces the time required for measurements.




Example of efficiency evaluation when inverter output is turned on in a cooking machine using induction heating

- GRAPHICAL POWER ANALYSIS**

The PZ4000 lets you analyze harmonics (up to 500th order) using high-speed sampling. With the FFT calculation function, you can perform spectrum analysis in the high-frequency range (up to 2.5 MHz). Analysis results are displayed on spectrum graphs. In addition, vectors showing the fundamental components of distorted waveforms can be displayed to give a visual presentation of the load balance in a 3-phase power supply system.

- Distorted wave power spectrum analysis**


With the PZ4000, you don't need a frequency analyzer to perform spectrum analysis on the carrier component of an inverter. Up to now, this type of analysis is difficult. A major advantage with the PZ4000 is that you can input signals directly without using probes. This removes any error due to probe tolerance.

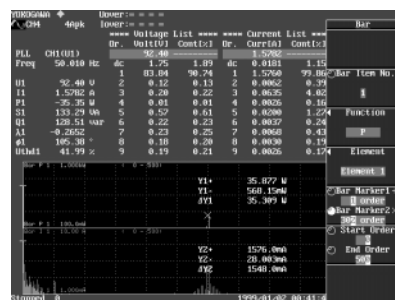

Example of spectrum analysis of current and power in inverter output

- The load balance evaluation in a three-phase equipment**

The vector display using the harmonic analysis function lets you visually know the condition of each phase in a 3-phase equipment. This makes evaluation simpler than when calculations are performed manually based on numerical data.

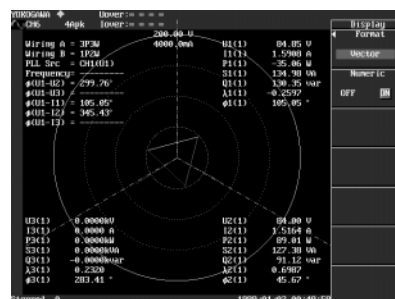


Example of fundamental wave vector display in inverter output


PZ4000

■ BASIC PERFORMANCE (Reference Values)


● Frequency characteristics (voltage and current)

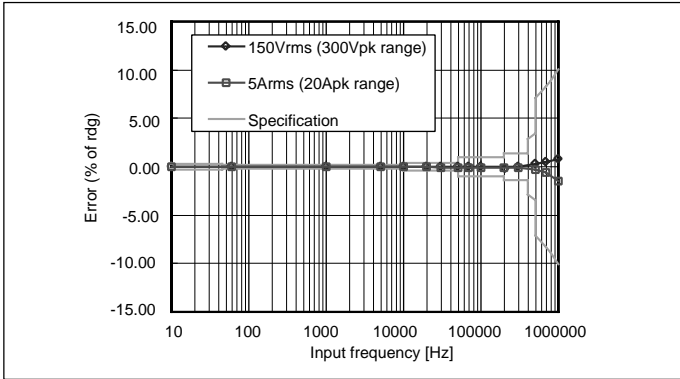


● Frequency characteristics (phase and zero power factor)

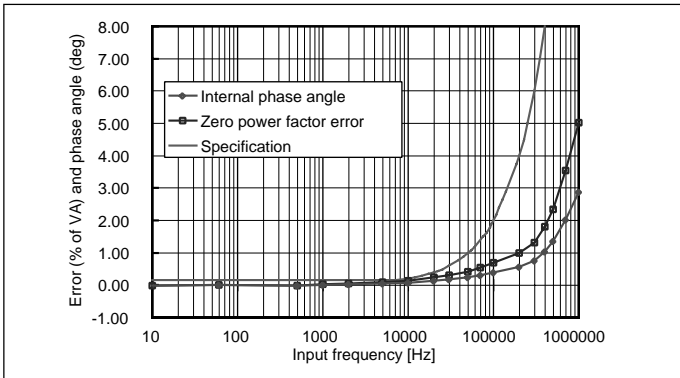

● Linearity (current input)

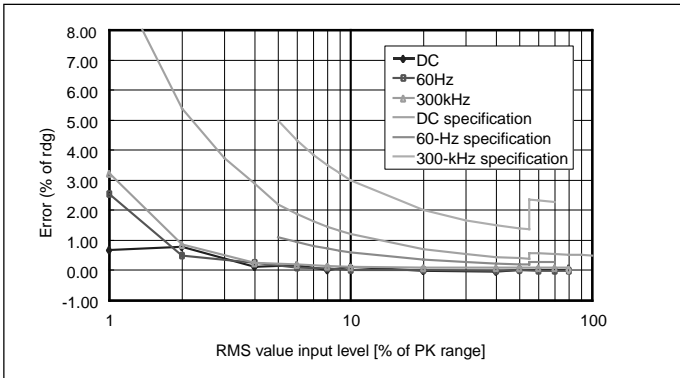

● Stability

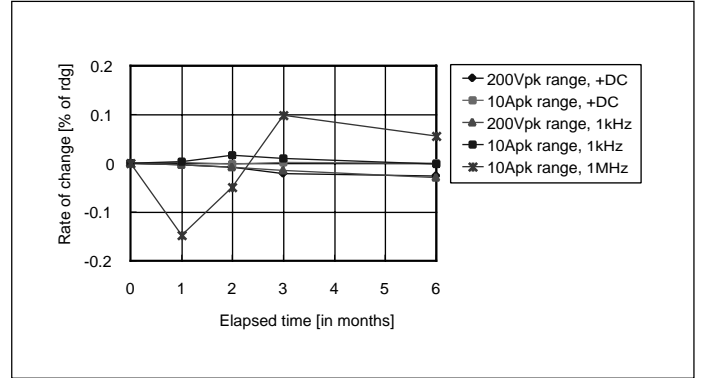

■ DIFFERENT MODULES FOR DIFFERENT USES

● 253751 Power measurement module:

Voltage direct input ranges: 30, 60, 120, 200, 300, 600, 1200, 2000 Vpk (1000 Vrms)

Current direct input ranges: 0.1, 0.2, 0.4, 1, 2, 4, 10 Apk (5 Arms)

Current sensor input ranges: 0.1, 0.2, 0.4, 1 Vpk (500 mVrms)

● 253752 Power measurement module:

Voltage direct input ranges: 30, 60, 120, 200, 300, 600, 1200, 2000 Vpk (1000 Vrms)

Current direct input ranges: 0.1, 0.2, 0.4, 1, 2, 4, 10 Apk (5 Arms, upper terminal)

1, 2, 4, 10, 20, 40, 100 Apk (20 Arms, lower terminal)

Current sensor input ranges: 0.1, 0.2, 0.4, 1 Vpk (500 mVrms)




■ SYNCHRONIZED MEASUREMENTS USING THE EXTER

● Synchronized measurements using multiple units (multiple channels) in a parallel connection

(Note: There is a maximum difference between PZ units of 3 microseconds plus two sample points.)



● Measurements synchronized with input waveform using external clock input

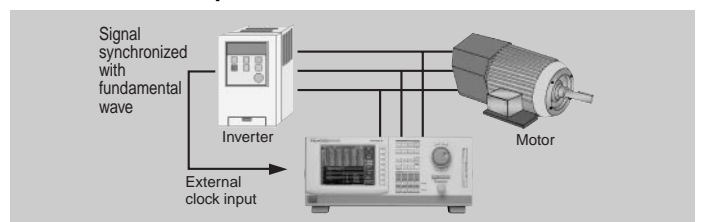

POWER MEASURING INSTRUMENTS



PZ4000

SPECIFICATIONS

Inputs

Type: Plug-in inputs

Slots: 4

Specifications (253751 and 253752 power measurement modules)

Input type	Voltage input	Current input
	Resistive voltage divider	Floating input Direct input: Shunt input External input: Resistive voltage divider
Rated values (ranges)	Direct inputs: 30, 60, 120, 200, 300, 600, 1200, 2000 Vpk (1000 Vrms)	Direct input 5 A: 0.1, 0.2, 0.4, 1, 2, 4, 10 Apk (5 Arms) Direct input 20 A: 1, 2, 4, 10, 20, 40, 100 Apk (20 Arms) External input: 100, 200, 400, 1000 mVpk (500 mVrms)
Input resistance	Input resistance: Approximately 1 MΩ Input capacitance: Approximately 5 pF	253751: Combination of direct input 5 A and external input 253752: Combination of direct inputs 5 A, 20 A, and external input
Instantaneous maximum allowable input (1 second)	Peak of 2000 V or rms of 1000 V (whichever is less)	Direct input 5 A: Peak of 30 A or rms of 15 A (whichever is less) Direct input 20 A: Peak of 150 A or rms of 40 A (whichever is less) External input: Peak and rms of 2 V or less
Continuous maximum allowable input	Peak of 2000 V or rms of 1000 V (whichever is less)	Direct input 5 A: Peak of 10 A or rms of 7 A (whichever is less) Direct input 20 A: Peak of 100 A or rms of 30 A (whichever is less) External input: Peak and rms of 2 V or less
Continuous maximum common mode voltage (50/60 Hz)	600 Vrms	
Common mode rejection ratio (600 Vrms)	Voltage input shorted and current input open 10 Hz ≤ f ≤ 1 kHz: ± 0.005% of range or less Other cases: Design value, ± (maximum range rating) / (range rating) × 0.0002 × f % of range or less (f is in kHz)	
Input terminal type	Plug-in terminal (safety terminal)	Direct input: Large binding post External input: BNC
A/D converter	Simultaneous voltage and current conversion, 12-bit resolution, maximum 5 MS/s sampling rate	
Line filter	Available cutoff frequencies: OFF, 500 Hz, 20 kHz, 1 MHz	
Zero-cross filter (for HF trigger and frequency detecting for averaging)	Available cutoff frequencies: OFF, 500 Hz, 20 kHz	
Range switching	Available settings for each element: Manual, Automatic, Remote Control	
Auto-range function	Range up: When input peak exceeds 80% of range rating Range down: When input peak falls to 15% or less of range rating	

Accuracy

Accuracy (253751 and 253752 power measurement modules)

	Voltage/current	Power
Accuracy Conditions	Temperature: 23°C ± 3°C Humidity: 50% ± 10% Input waveform: Sine-wave Common mode voltage: 0 V Power factor: cosφ = 1 Within 3 months after calibration * DC accuracy is specified with NULL function on and line filter (1 MHz) on. * For at least five input signal cycles in observation time, and at least 10 k words of sampling data	
Frequencies		
DC	±(0.2% of rdg + 0.1% of rng)	±(0.2% of rdg + 0.1% of rng)
0.1 Hz ≤ f < 10 Hz	±(0.2% of rdg + 0.1% of rng)	±(0.2% of rdg + 0.05% of rng)
10 Hz ≤ f < 45 Hz	±(0.2% of rdg + 0.05% of rng)	±(0.2% of rdg + 0.025% of rng)
45 Hz ≤ f ≤ 1 kHz	±(0.1% of rdg + 0.05% of rng)	±(0.1% of rdg + 0.025% of rng)
1 kHz < f ≤ 10 kHz	±(0.1% of rdg + 0.05% of rng)	±(0.1% of rdg + 0.04% of rng)
10 kHz < f ≤ 50 kHz	±(0.2% of rdg + 0.1% of rng)	±(0.2% of rdg + 0.05% of rng)
50 kHz < f ≤ 100 kHz	±(0.6% of rdg + 0.2% of rng)	±(0.6% of rdg + 0.1% of rng)
100 kHz < f ≤ 200 kHz	±(0.6% of rdg + 0.2% of rng)	±(1.5% of rdg + 0.15% of rng)
200 kHz < f ≤ 400 kHz	±(1% of rdg + 0.2% of rng)	±(1.5% of rdg + 0.15% of rng)
400 kHz < f ≤ 500 kHz	±[(0.1 + 0.006 × f)% of rdg + 0.2% of rng]	±[(0.1 + 0.009 × f)% of rdg + 0.15% of rng]
500 kHz < f ≤ 1 MHz	±[(0.1 + 0.006 × f)% of rdg + 2% of rng]	±[(0.1 + 0.009 × f)% of rdg + 1.5% of rng]
1 MHz < f ≤ 5 MHz	±[(0.1 + 0.006 × f)% of rdg + 2% of rng]	—
Additional error	10 Hz and below and 1 MHz and above are design values (1 MHz and above applies only to voltage inputs and external current sensor inputs). When input is voltage input of 400 Vrms or greater: Add [(reading error) × 1.5 × U ² % of rdg]. In addition, values of 100 kHz or greater are design values; add [(reading error) × 0.005 × f × U ² % of rdg]. When input is 10 Arms or greater in module 253752: Add [(reading error) × 0.0002 × I ²]. Units U (input voltage): kV, I (input current): A, f (frequency): kHz	
Power factor influence (f is in kHz)	For cosφ = 0.45 to 66 Hz: Add 0.15% of apparent power reading to the above accuracy. Other frequencies: design values Add (0.02 of apparent power reading × f%) to the above accuracy (assumes apparent power reading of 0.15% or higher) For 0 < cosφ < 1 45 to 66 Hz: Add [(0.15 × tanφ)% of rdg] to the above accuracy. Other frequencies: design values Add [(0.02 × f × tanφ)% of rdg] to the above accuracy (assumes 0.15 × tanφ% of rdg or higher)	
One year accuracy	Reading error (3 months accuracy) + range error (3 months accuracy) × 1.5	
Line filter effects	Add 0.5% of rdg with fc/10.	Add 1% of rdg with fc/10.

Effective input range	As per the above accuracy when the input signal is a sine wave with rms at 5 to 55% of range rating, or when the input signal is DC between -55% and 55% of measurement range. Double the above 3 months reading error when the input signal is a sine wave with rms at 55 to 70% of range rating, or when the input signal is DC between -100% and -55% or between 55% and 100% of measurement range.
Temperature coefficient	Add 0.01% of rdg/°C (5 to 20°C, 26 to 40°C, but 10 kHz or less)

Accuracy per sampling (instantaneous value) during cursor measurement: ±2% of rng (design value) (does not include error relating to analog bandwidth or sampling resolution)
Measurement accuracy when there are less than five input cycles and sampled data are less than 10 k words: (1/10 of reading error) × (5/(number of input signal cycles in observation time)) × (10 k words/ (number of sampled data words))
Add % of rdg to 3 months accuracy (design value)
We recommend storing the PZ4000 at temperatures of 40°C or less to ensure measurements within the above accuracy specifications.

Numerical calculations

Sigma calculation formulas for different wiring types

	Single phase, 3 wires	3 phases, 3 wires	3V3A	3 phases, 4 wires
U (voltage) Ui	(U1 + U2)/2		(U1 + U2 + U3)/3	
I (current) li	(I1 + I2)/2		(I1 + I2 + I3)/3	
P (active power) P	P1 + P2			P1 + P2 + P3
Q (reactive power)				
Normal measurement	Qi = √(Si ² - Pi ²)		Q1 + Q2	
Harmonic measurement	Qi		Q1 + Q2 + Q3	
S (apparent power)				
Normal measurement	Si = Ui × li	S1 + S2	√3/2 (S1 + S2)	√3/3 (S1 + S2 + S3)
Harmonic measurement	S = √(P ² + Q ²)	√(ΣP ² + ΣQ ²)		
λ (power factor) P/S	ΣP/ΣS			
φ (phase angle) cos ⁻¹ (P/S)	cos ⁻¹ (ΣP/ΣS)			

Wiring settings: Divisible into two groups

Setting	ΣA		ΣB		Number of attached elements
	Used elements	Setting	Used elements	Setting	
1P2W (single phase, 2 wires)	1	—	—	—	1 element or more
	1	1P2W (single phase, 2 wires)	2	—	2 element or more
	1	1P3W (single phase, 3 wires)	2, 3	—	3 element or more
	1	3P3W (3 phases, 3 wires)	2, 3	—	3 element or more
1P3W (single phase, 3 wires)	1,2	—	—	—	2 element or more
	1,2	1P2W (single phase, 2 wires)	3	—	3 element or more
	1,2	1P3W (single phase, 3 wires)	3, 4	—	4 element or more
	1,2	3P3W (3 phases, 3 wires)	3, 4	—	4 element or more
3P3W (3 phases, 3 wires)	1,2	—	—	—	2 element or more
	1,2	1P2W (single phase, 2 wires)	3	—	3 element or more
	1,2	1P3W (single phase, 3 wires)	3,4	—	4 element or more
	1,2	3P3W (3 phases, 3 wires)	3,4	—	4 element or more
3V3A (3 phases, 3 wires)	1,2,3	—	—	—	3 element or more
	1,2,3	1P2W (single phase, 2 wires)	4	—	4 element or more
3V4W (3 phases, 4 wires)	1,2,3	—	—	—	3 element or more
	1,2,3	1P2W (single phase, 2 wires)	4	—	4 element or more

POWER MEASURING INSTRUMENTS



PZ4000

Calculation display resolution

	P (active power)	Q (reactive power)	S (apparent power)	λ (power factor)	ϕ (phase angle)
Display range	Ratings depend on the voltage and current ranges.	Ratings depend on the voltage and current ranges. ($Q \geq 0$)	Ratings depend on the voltage and current ranges.	-1 to 0 to 1	LEAD180 to 0 to LAG180 Or 0 to 360
Maximum display or maximum resolution	99999 or 999999 (selectable)	99999 or 999999 (selectable)	99999 or 999999 (selectable)	± 1.0000	0.01

Note 1: The apparent power (S), reactive power (Q), power factor (λ), and phase angle (ϕ) for the PZ4000 are calculated based on voltage, current, and active power. (However, reactive power is measured directly during harmonic measurement.) Therefore, during distorted wave input, there may be a difference between these values and those of other measuring instruments based on different measurement principles.

Note 2: If either the voltage or current is 0.25% or less of the range rating, zero will be displayed for the apparent power (Q) and reactive power (S), and errors will be displayed for the power factor (λ) and phase angle (ϕ).

Note 3: If both the voltage and current are sinewaves, and there is not a great difference between voltage and current in terms of the ratio of input to measurement range, then the lead/lag phase angle ϕ will be correctly detected.

Note 4: There are no accuracy specifications for 0 and 180 ± 5 degrees when phase angle reading is 0 to 360.

Measurement function items:

U (voltage), I (current), P (active power), S (apparent power), Q (reactive power), λ (power factor), ϕ (phase angle), CF (crest factor), FF (form factor), $|Z|$ (impedance), R_s and R_p (resistance), X_s and X_p (reactance), η and $1/\eta$ (efficiency), P_c (Corrected Power), F1 to F4 (user-defined functions)

Delta computation (during normal measurement only):

Calculated by taking the sum or difference of instantaneous voltage and current values. One of the following can be selected.

Measurement parameters: ΔU_{rms} , ΔU_{mn} , ΔU_{dc} , ΔU_{ac} , ΔI_{rms} , ΔI_{mn} , ΔI_{dc} , ΔI_{ac}

u1-u2: Voltage only

i1-i2: Current only

3-phase 3-wire/3V3A conversion

Y- Δ conversion: Phase voltage-line voltage conversion, neutral line current

Δ -Y conversion: Line voltage-phase voltage conversion, neutral line current

Waveform calculations

Parameters	Voltage and current of any element
Waveform calculations	2 types (MATH1 and MATH2)
ITEM	C1 to C8: CH1 to CH8 data
Memory size	100 k words (if MATH1 and MATH2 are both used, then 100 k words each)
Arithmetic calculations	Addition, subtraction, multiplication, division
Special functions	AVG () Exponential average of instantaneous values TREND () Average data for individual cycles Root mean square values when C1 to C8 are inserted (voltage and current) Power average values (power) for C1*C2, C3*C4, C5*C6, and C7*C8. Only the following can be set in the parentheses: one item, C1*C2, C3*C4, C5*C6, or C7*C8. (Functions cannot be entered in parentheses.) Other functions: ABS, SQR, SQRT, LOG, LOG10, EXP, NEG, TINTG

FFT

Type	PS (power spectrum)
Number of points	1000 points, 2000 points, 10000 points
Window functions	Rectangular, Hanning
Measured parameters	Voltage and current rms values, active power
Starting point can be specified.	

Frequency measurements

Measurement type	Reciprocal
Measured parameters	Voltage and current values of all installed power measurement modules (only channels set to SYNC source during harmonic analysis).
Maximum display	99999 (2.5000 MHz max)
Accuracy	For observation period of 2 ms or longer $10 \text{ Hz} \leq f < 10 \text{ kHz}$ $\pm 0.1\%$ of rdg + 1 digit Assumes sinewave with input of at least 15% of range; 5 cycles or more within observation period; and measured frequency no greater than 1/2.5 of sampling rate.
Frequency measurement filter	Set using zero-cross filter.

Harmonic measurement

Measurement type	PLL synchronization
Measured frequency range	Fundamental wave frequency range of 20 Hz to 6.4 kHz

Measured function items:

U, I, P, S, Q, λ , ϕ (between V and A) for each order, ϕU , ϕI (phase difference for harmonic component relative to fundamental wave), $|Z|$, R_s , R_p , X_s , X_p , TOTAL U, I, P, S, Q, λ (Σ calculation possible), and ϕ
U, I, and P harmonic distortion factor of each order
U, I, and P THD
PLL synchronization frequencies
UTHF (voltage telephone harmonic factor), ITHF (current telephone harmonic factor), UTIF (voltage telephone influence factor), ITIF (current telephone influence factor), HVF (harmonic voltage factor), HCF (harmonic current factor)

Set record length

Same as normal.

FFT data points

8192
FFT analysis data starting point in acquisition memory can be set as desired.

FFT processing word length

32 bits

Window function

Rectangular

PLL synchronization options

Either external clock or voltage/current in all installed power measurement modules can be selected. external clock can also be used without PLL. When this is done, the fundamental frequency is 1/4096 of the external clock.

PLL synchronization filter

Set using zero-cross filter.

Anti-aliasing filter

Set using line filter ($f_c = 20 \text{ kHz}$)

Relationships between sampling rate, window width, and number of analysis orders

Fundamental frequency (Hz)	Sampling rate (Hz)	Window width	Maximum number of analysis orders	Maximum number of analysis orders with accuracy equal to normal measurement accuracy
$20 \text{ Hz} \leq f < 40 \text{ Hz}$	$f \times 4096$	2	500	50
$40 \text{ Hz} \leq f < 80 \text{ Hz}$	$f \times 2048$	4	500	50
$80 \text{ Hz} \leq f < 160 \text{ Hz}$	$f \times 1024$	8	500	50
$160 \text{ Hz} \leq f < 320 \text{ Hz}$	$f \times 512$	16	200	25
$320 \text{ Hz} \leq f < 640 \text{ Hz}$	$f \times 256$	32	100	25
$640 \text{ Hz} \leq f < 1.28 \text{ kHz}$	$f \times 128$	64	50	10
$1.28 \text{ kHz} \leq f < 2.56 \text{ kHz}$	$f \times 64$	128	30	10
$2.56 \text{ kHz} \leq f < 6.4 \text{ kHz}$	$f \times 32$	256	15	-

Note 1: Hysteresis is applied across each of the above fundamental frequency bands.

Measurement accuracy

Accuracy for bands where normal measurement accuracy is not applied: Add $[0.001 \times f \times (\text{order number})\% \text{ of reading}]$ (design value) Where f (in kHz) is the frequency for that order.

Display

Display	6.4-inch color TFT liquid crystal display
Pixel area for full display	640×480 (The liquid crystal display may contain approximately 0.02% defects among all display pixels.)
Pixel area for waveform	501×432
Display area	Numerical Normal measurement: 8 values values, 16 values, 42 values, 78 values, ALL Harmonic measurement: 8 values, 16 values, Single List, Dual List, Σ List
Waveforms	Single, Dual, Triad, Quad
Vector	Phase diagram for fundamental component during harmonic measurement
Bar	Bar graph up to maximum number of analysis orders during harmonic measurement
Simultaneous display	Numerical value + waveform, numerical value + bar, waveform + bar
Alarm display	Displayed on screen (only sensed during observation period). Peak over: When instantaneous value exceeds approximately 125% of range
Maximum number of waveform display traces	24 traces (during zooming): 8 captured waveforms + 16 zoomed waveforms
Display updating cycle	Depends on the observation time and record length. The display updating cycle is approximately 2 seconds in normal measurement mode, using a 100 ms observation time, 100 k word record length setting, and 8 channels, with numerical value calculation ON and waveform calculation off. The display updating cycle is approximately 2 seconds in harmonic measurement mode, using a 100 ms observation period, 100 k word record length setting, and 8 channels, with numerical value calculation ON and waveform calculation off.

Memory

Set record length	100 k word/CH (standard), 1 M word/CH (with /M1 option), 4 M word/CH (with /M3 option)
Record length settings	100 k word, 1 M word, 4 M word (or 50 k word, 500 k word, and 2 M word when record length is divided; screen data are saved and measurement is ended when the STOP button is pressed) The sampling rate is selected automatically when the record length and observation time are set.

Triggers

Modes	Off, Auto, Auto Level, Normal, and (with edge trigger) HF Auto, HF Normal
Types	Edge, window
Sources	INT (channels 1 through 8), and (with edge trigger) EXT
Slopes	Rising, falling, both
Trigger position	0% to 100% HF cutoff frequency: set using zero-cross filter. When HF is selected as the trigger mode, the trigger level cannot be set.

POWER MEASURING INSTRUMENTS



PZ4000

Screen data output and saving (copying)

Internal printer (optional) Screenshot hard copies
 Floppy disks and external SCSI devices (optional) Formats: PostScript, TIFF, BMP
 Centronics port Formats: ESC-P, ESC-P2, LIPS3, PR201, PCL5, BJ

External I/O

EXT TRIG IN (external trigger input)

Connector BNC
 Input voltage CMOS level (L: 0 to 1 V, H: 4 to 5 V)
 Minimum pulse width 1 μ s
 Trigger delay time (2 μ s + 1 sample cycle) or less

EXT TRIG OUT (external trigger output)

Connector BNC
 Input voltage CMOS level (L: 0 to 1 V, H: 4 to 5 V)
 Output delay time (1 μ s + 1 sampling cycle) or less
 Output holding time Low level 200 ns or longer

EXT CLK (external sampling clock input)

Connector BNC
 Input voltage CMOS level (L: 0 to 1 V, H: 4 to 5 V)
 Input frequency range 1 kHz to 250 kHz (50% duty)
 20 Hz to 6.4 kHz when used as PLL source for harmonic analysis. 4096 times the fundamental frequency when used as a sampling clock for harmonic analysis. (The external clock is internally sampled at 20 MHz.)

Internal floppy drive

Size 3.5 inches
 Formats 640 KB, 720 KB, 1.2 MB, 1.44 MB

GPIB port

Electrical and mechanical specifications
 Compliant with IEEE Standard 488-1978.
 Functional specifications SH1, AH1, T6, L4, SR1, RL1, PP0, DC1, DT0, C0
 Protocol Compliant with IEEE Standard 488.2 1987.

Serial (RS-232) port

Connector D-Sub 9-pin
 Standard EIA-574 standard (for EIA-232 (RS-232) standard 9-pin connector)
 Bit rates 1200, 2400, 4800, 9600, 19200 bps

Centronics port

Connector D-Sub 25-pin

SCSI port (optional)

Standard Small Computer System Interface (SCSI) ANSI X3.131-1986
 Connector Half-pitch 50-pin (pin type)
 Connector pin assignment Unbalanced (single-end), built-in terminator
 Usable hard drives SCSI hard drives, NEC MS-DOS Ver. 3.3 or higher, or EZ-SCSI drives that are formattable.
 Usable MO drives Drive capacities up to 640 MB are supported.
 Other drive types ZIP and PD drives can be used.
 For further information, please contact your nearest YOKOGAWA dealer.

General specifications

Warmup time Approximately 30 minutes
 Operating temperature and humidity ranges 5 to 40°C, 20 to 85% RH (or 35 to 80% when using printer), no condensation
 Storage temperature range -25 to 60°C, no condensation Avoid storing the product for extended periods of time in hot and humid environments. Doing so may adversely affect performance.
 Maximum operating altitude 2000 meters
 Insulating resistance 50 M Ω or greater at 500 V DC
 253710 Between case and power plug
 253751, 253752 Between voltage input terminals and case Between current input terminals and case Between voltage input terminals and current input terminals
 Withstand voltage 1500 V for one minute at 50/60 Hz.
 253710 Between case and power plug: 1500 V for one minute at 50/60 Hz.
 253751, 253752 Between voltage input terminals and case, and between current input terminals and case: 2200 V for one minute at 50/60 Hz
 Between voltage input terminals and current input terminals : 3700 V for one minute at 50/60 Hz
 Rated supply voltages 100 to 120 V AC, 200 to 240 V AC (switching not required)
 Allowed supply voltage fluctuation ranges 90 to 132 V AC, 180 to 264 V AC
 Rated supply frequencies 50/60 Hz
 Allowed supply frequency fluctuation range 48 to 63 Hz
 Consumed power Approximately 200 VA (when using printer)
 External dimensions Approximately 426 (W) \times 177 (H) \times 450 (D) mm (including 253710 printer cover; does not include knobs and projections)
 Weight Approximately 15 kg (main unit with four 253752 power measurement modules installed)

Recording

Built-in printer (optional)

Printing method Thermal line-dot printing
 Dot density 8 dot/mm
 Paper width 112 mm
 Effective recording width 104 mm
 Recording speed Maximum 20 mm/s

AVAILABLE MODELS

Main unit

Model	Suffix Code	Description
253710		PZ4000 Power Analyzer
Power cord	-D	UL/CSA Standard
	-F	VDE Standard
	-R	SAA Standard
	-Q	BS Standard
Options	/M1	Memory extension to 1 M word/CH
	/M3	Memory extension to 4 M word/CH
	/B5	Built-in printer
	/C7	SCSI interface

Plug-in modules

Model	Suffix Code	Description
253751		Power measurement module Voltage: 1000 V Current: 5 A Current sensor: 500 mV
253752		Power measurement module Voltage: 1000 V Current: 5 A and 20 A Current sensor: 500 mV
Module specifications	-E1	Plug-in unit


Accessories (sold separately)

Product	Model or part number	Description	Order quantity
Rack mounting kit	751535-E4	For EIA	1
Rack mounting kit	751535-J4	For JIS	1
BNC cable	366924	BNC cable BNC-BNC, 1 m	1
BNC cable	366925	BNC cable BNC-BNC, 2 m	1
BNC cable	366926	BNC-alligator clip cable	1
Conversion adapter	366971	9-pin*1/25-pin*2 conversion adapter	1
Measurement lead	758917	75 cm, two leads (red and black) in a set	1
Fork terminal adapter set	758921	4 mm fork terminal, banana terminal conversion, red and black (one each)	1
Alligator clip adapter (rated for 300 V)	758922	Banana-alligator conversion, two in a set	1
Alligator clip adapter (rated for 1000 V)	758929	Banana-alligator conversion, two in a set	1
Fuse	A1354EF	250 V, 6.3 Arms, time lag 100 V/200 V common	2
Input cable	B9284LK	For external input, 50 cm	1
Current input protective cover	B9315DJ	Acrylic current input protective cover	1
Printer roll chart	B9850NX	Thermal paper, 30 meters (one roll equals one unit)	5

*1: EIA-574 standard

*2: EIA-232 standard (RS-232)

DIMENSIONS

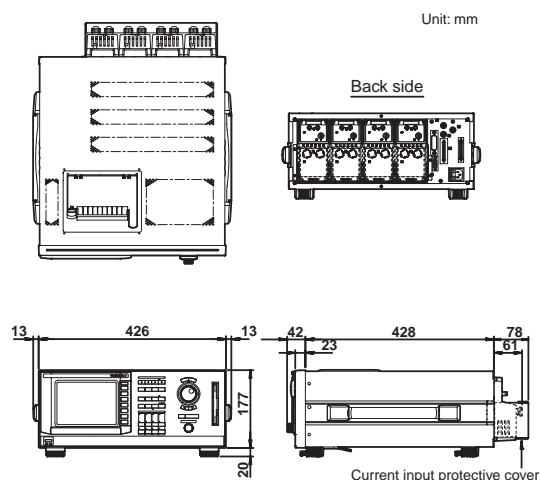

Unless otherwise indicated, tolerance for dimensions is $\pm 3\%$ (or ± 0.3 mm for less than 10 mm).